

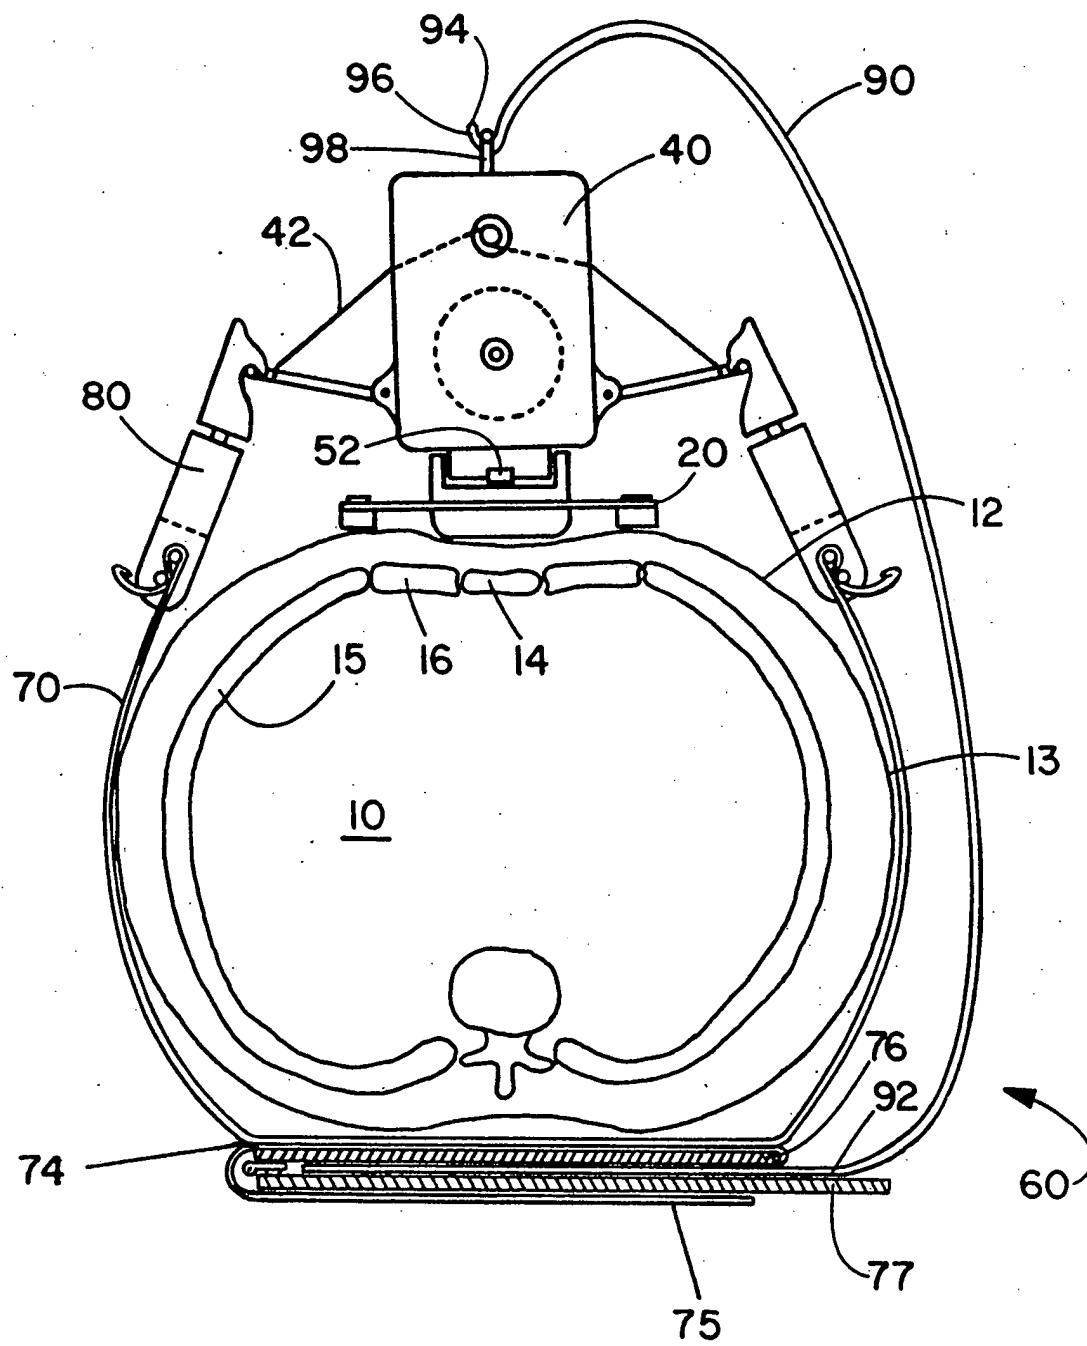


FIG 1

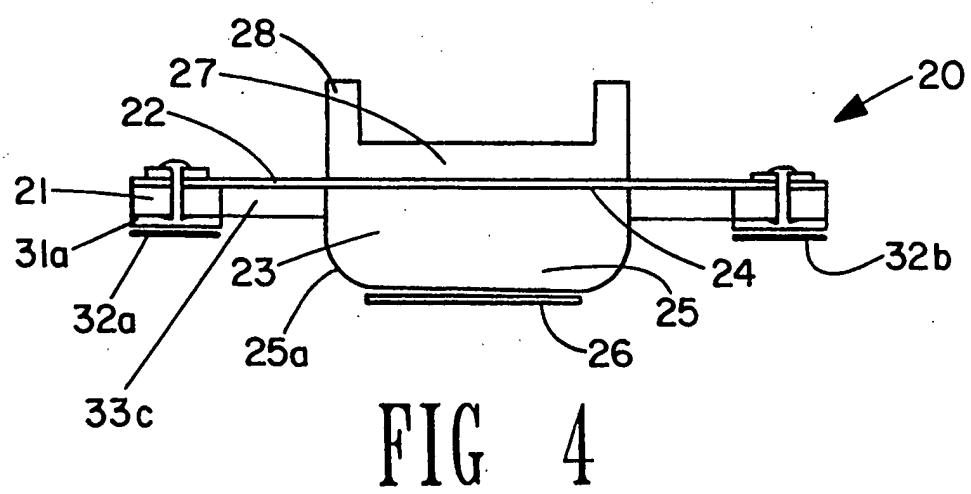

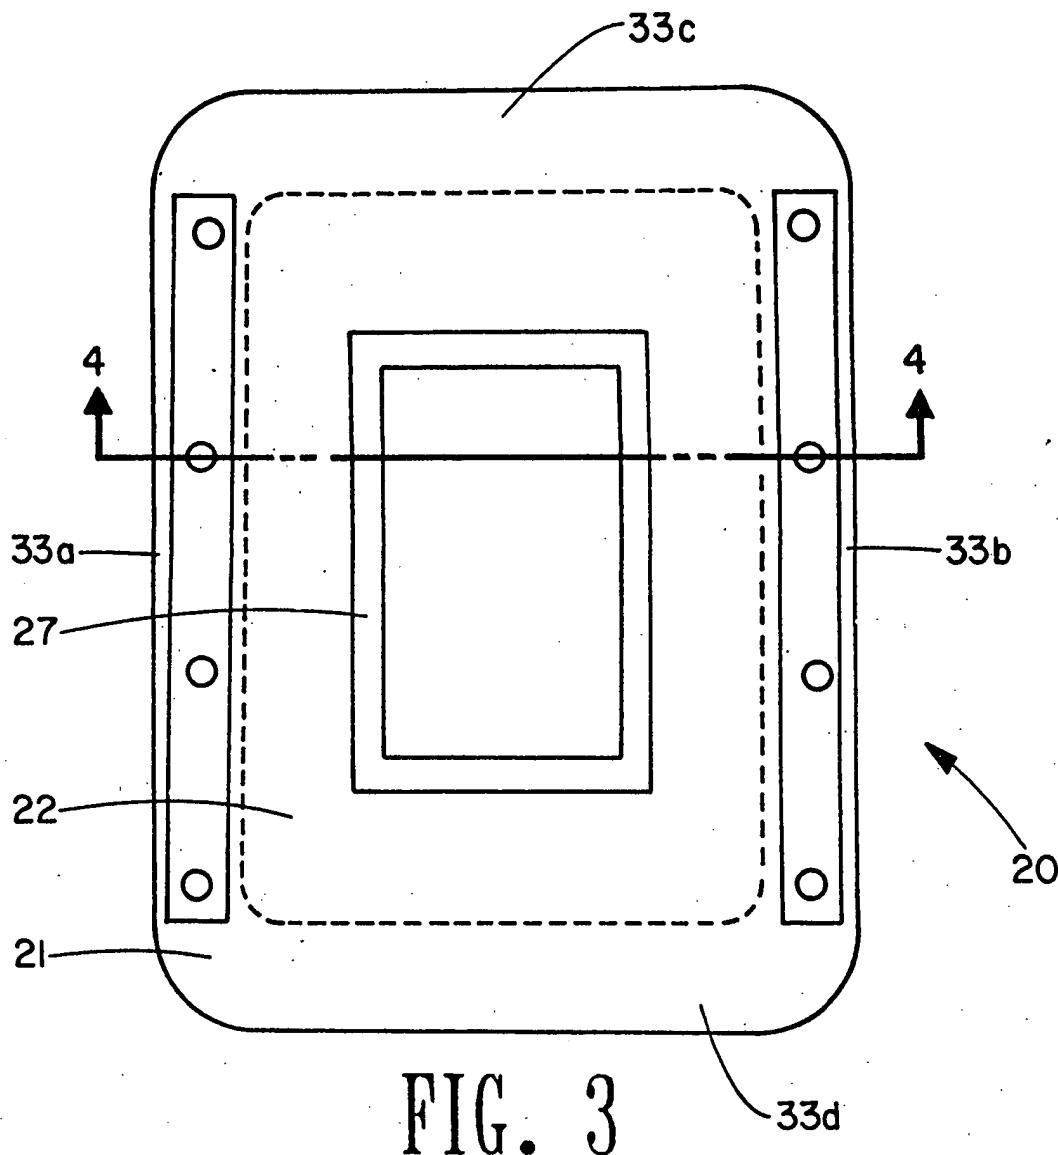

4/15

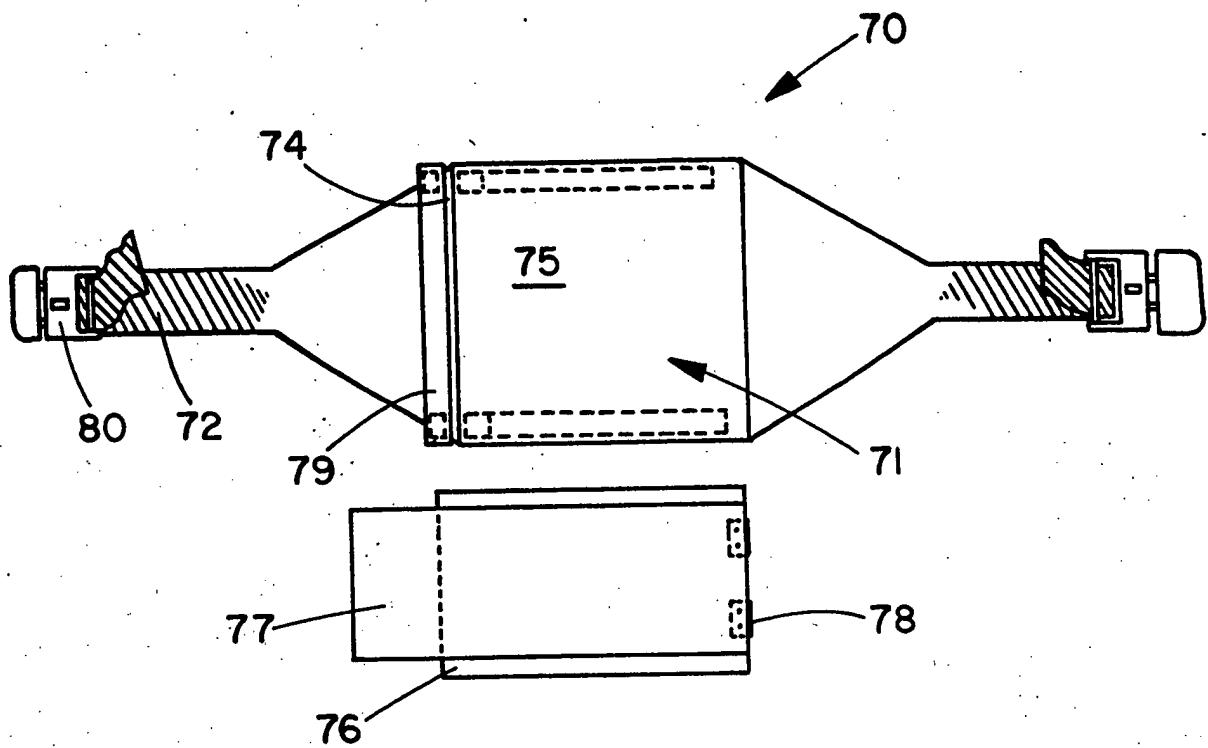


FIG. 5

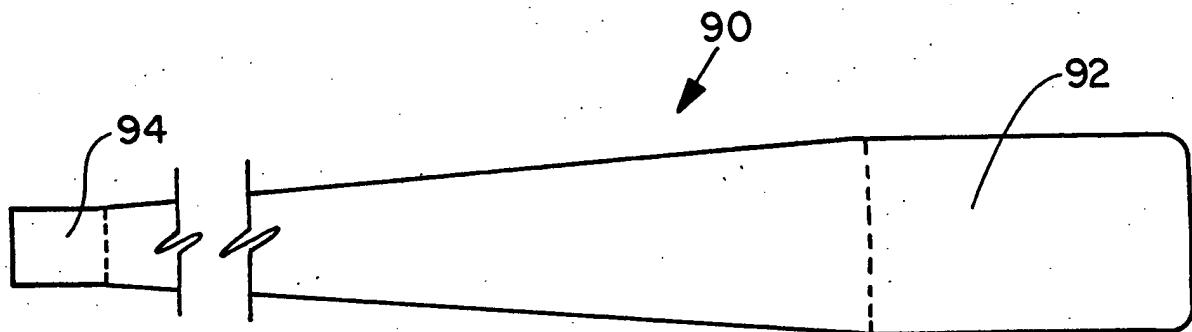


FIG 6

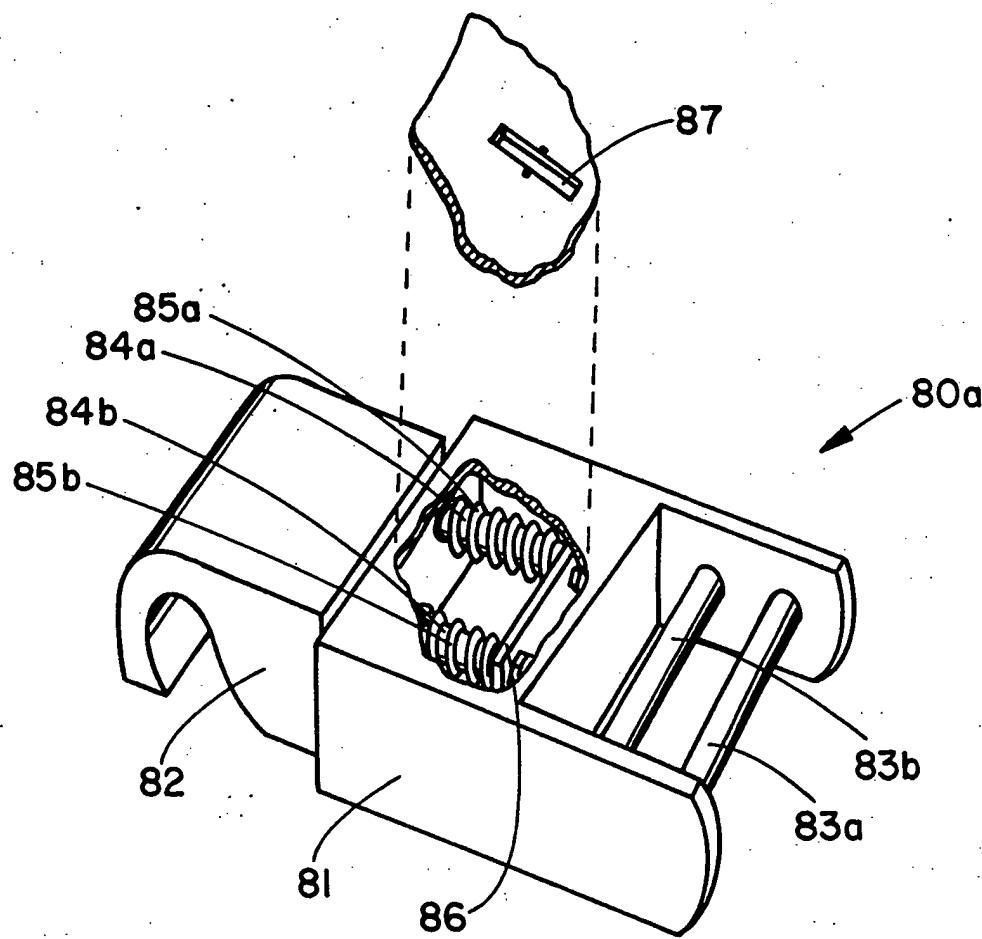


FIG. 7

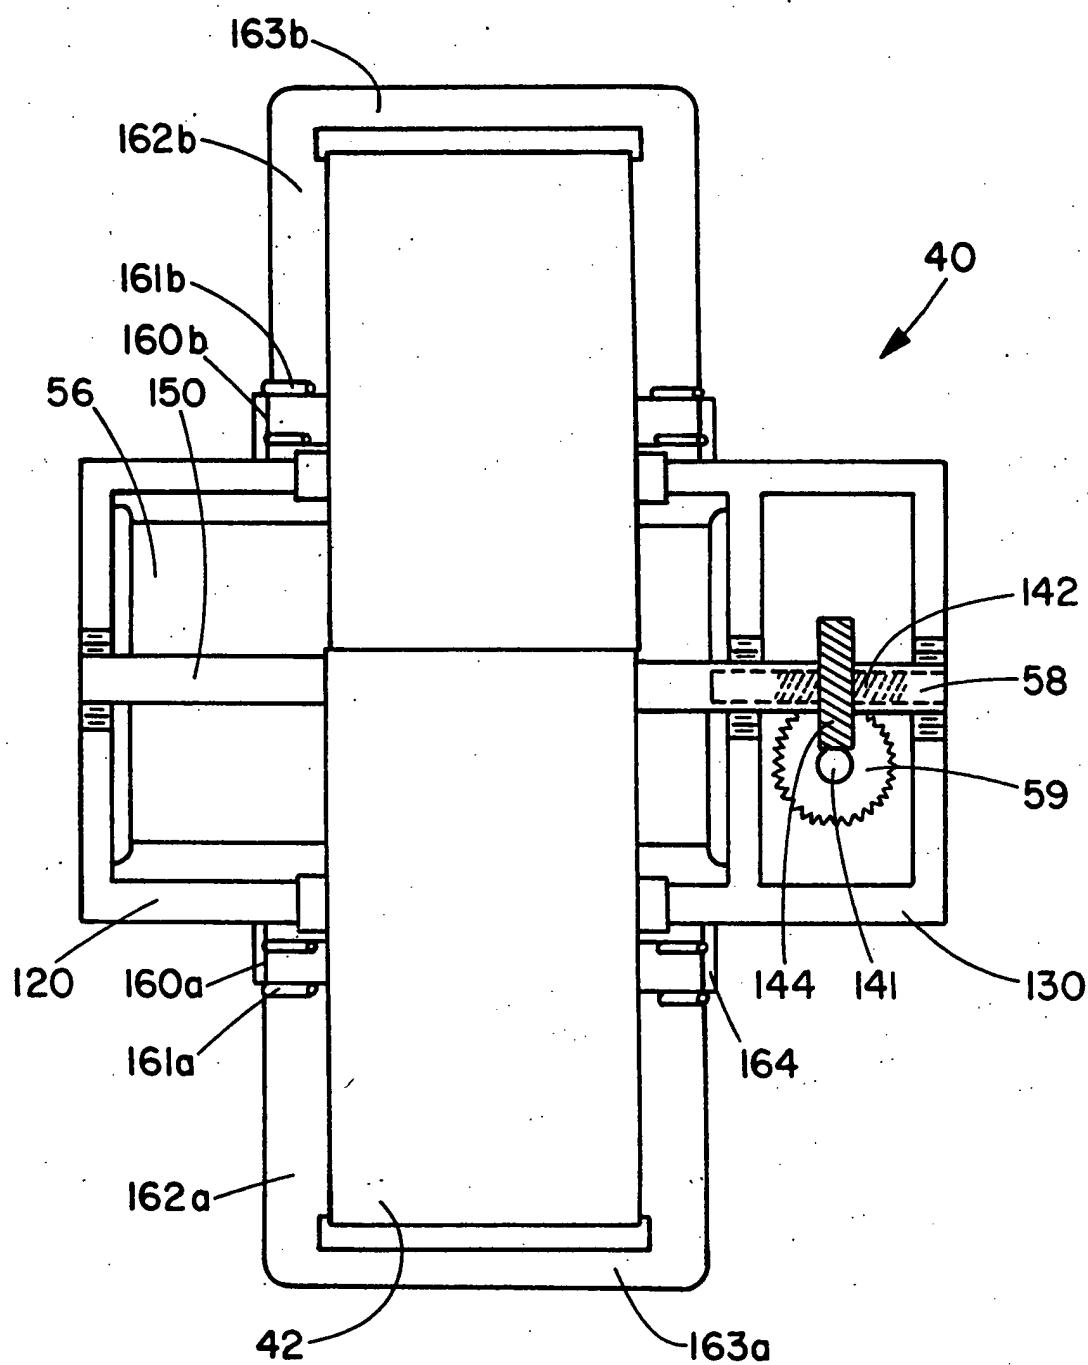


FIG 8

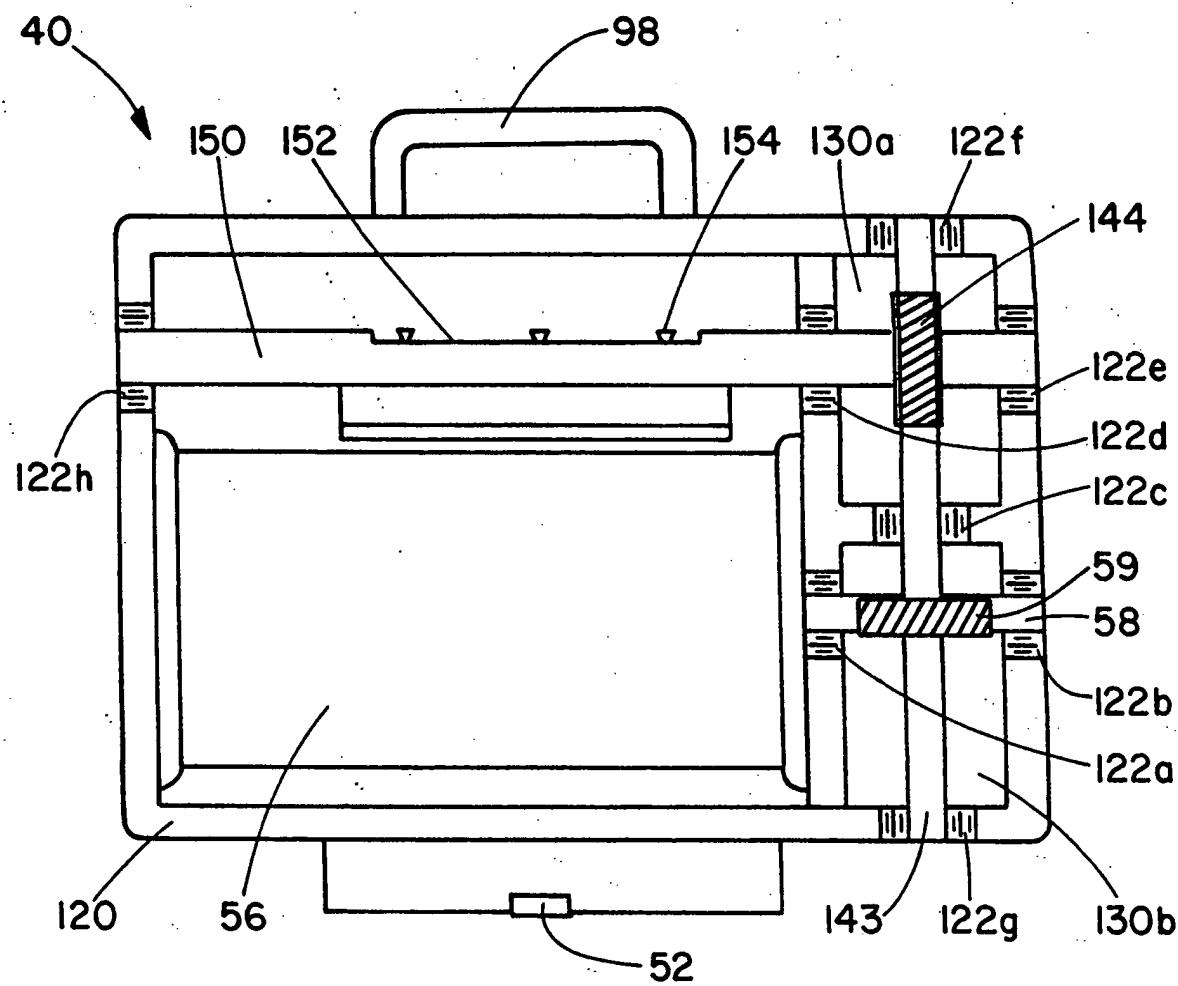


FIG. 9

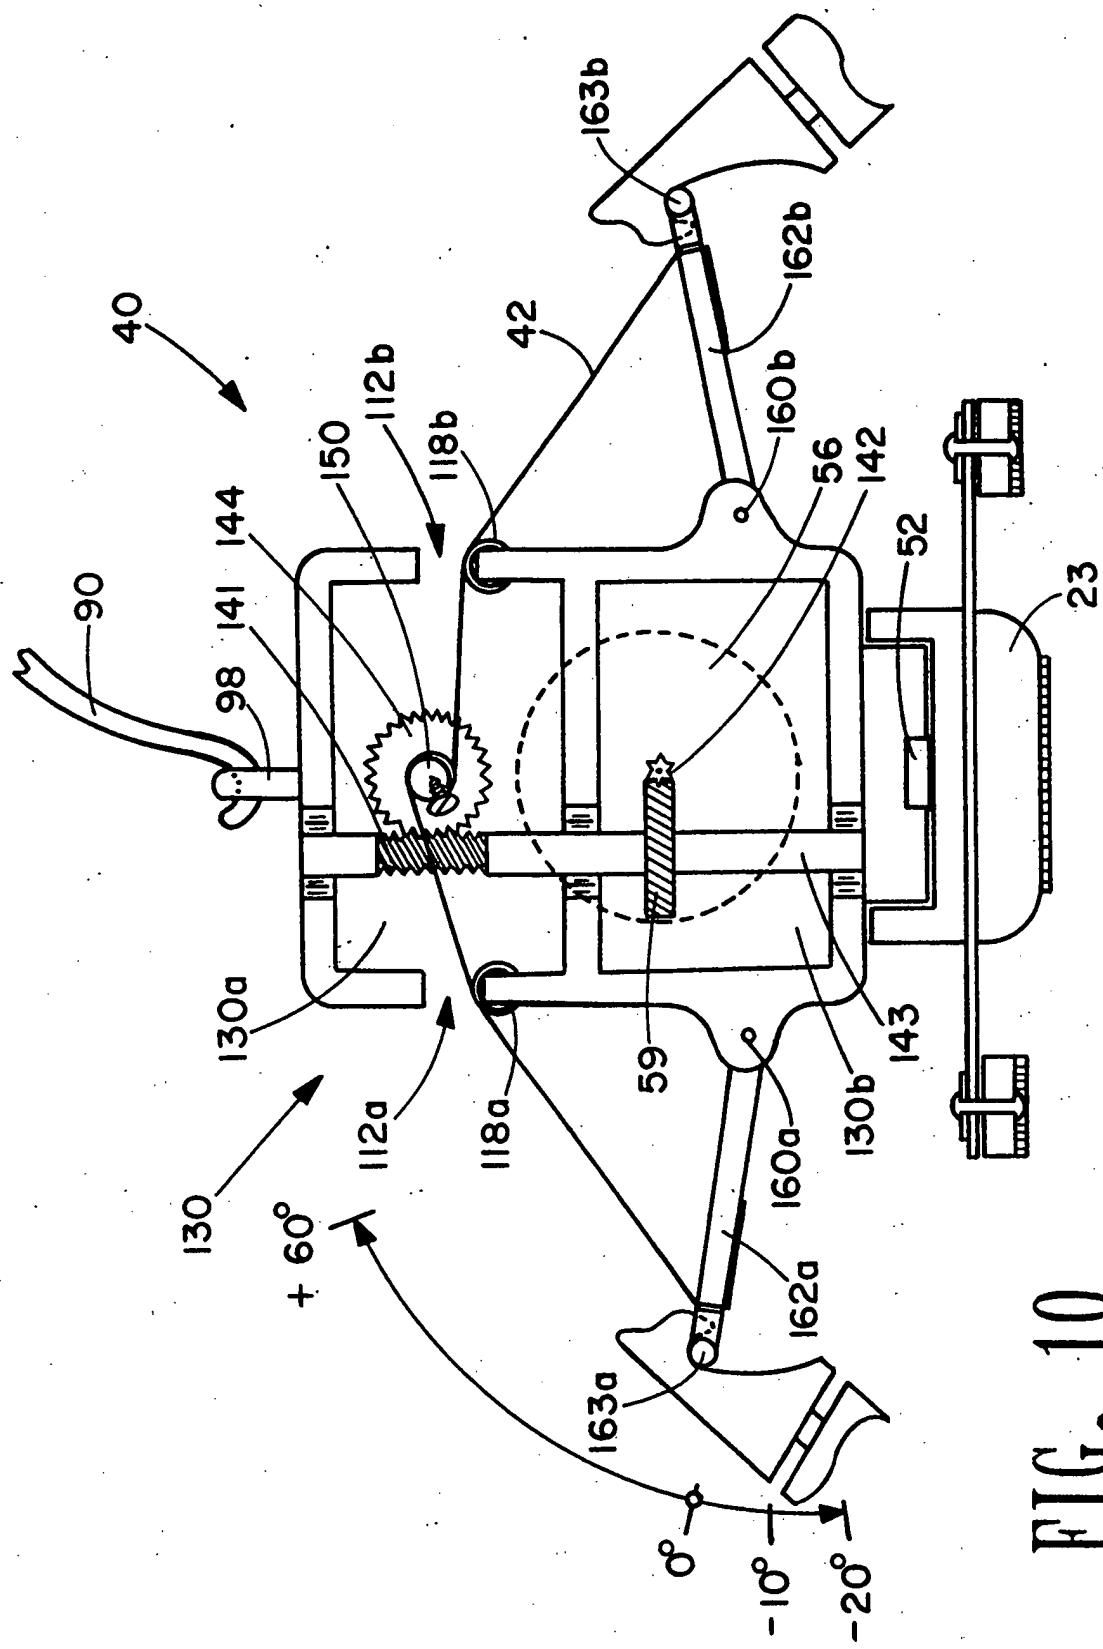


FIG. 10

9/15

CONTROL DIAGRAM FOR COMPACT TRAMPOLINE CPR  
SYSTEM (TCP)

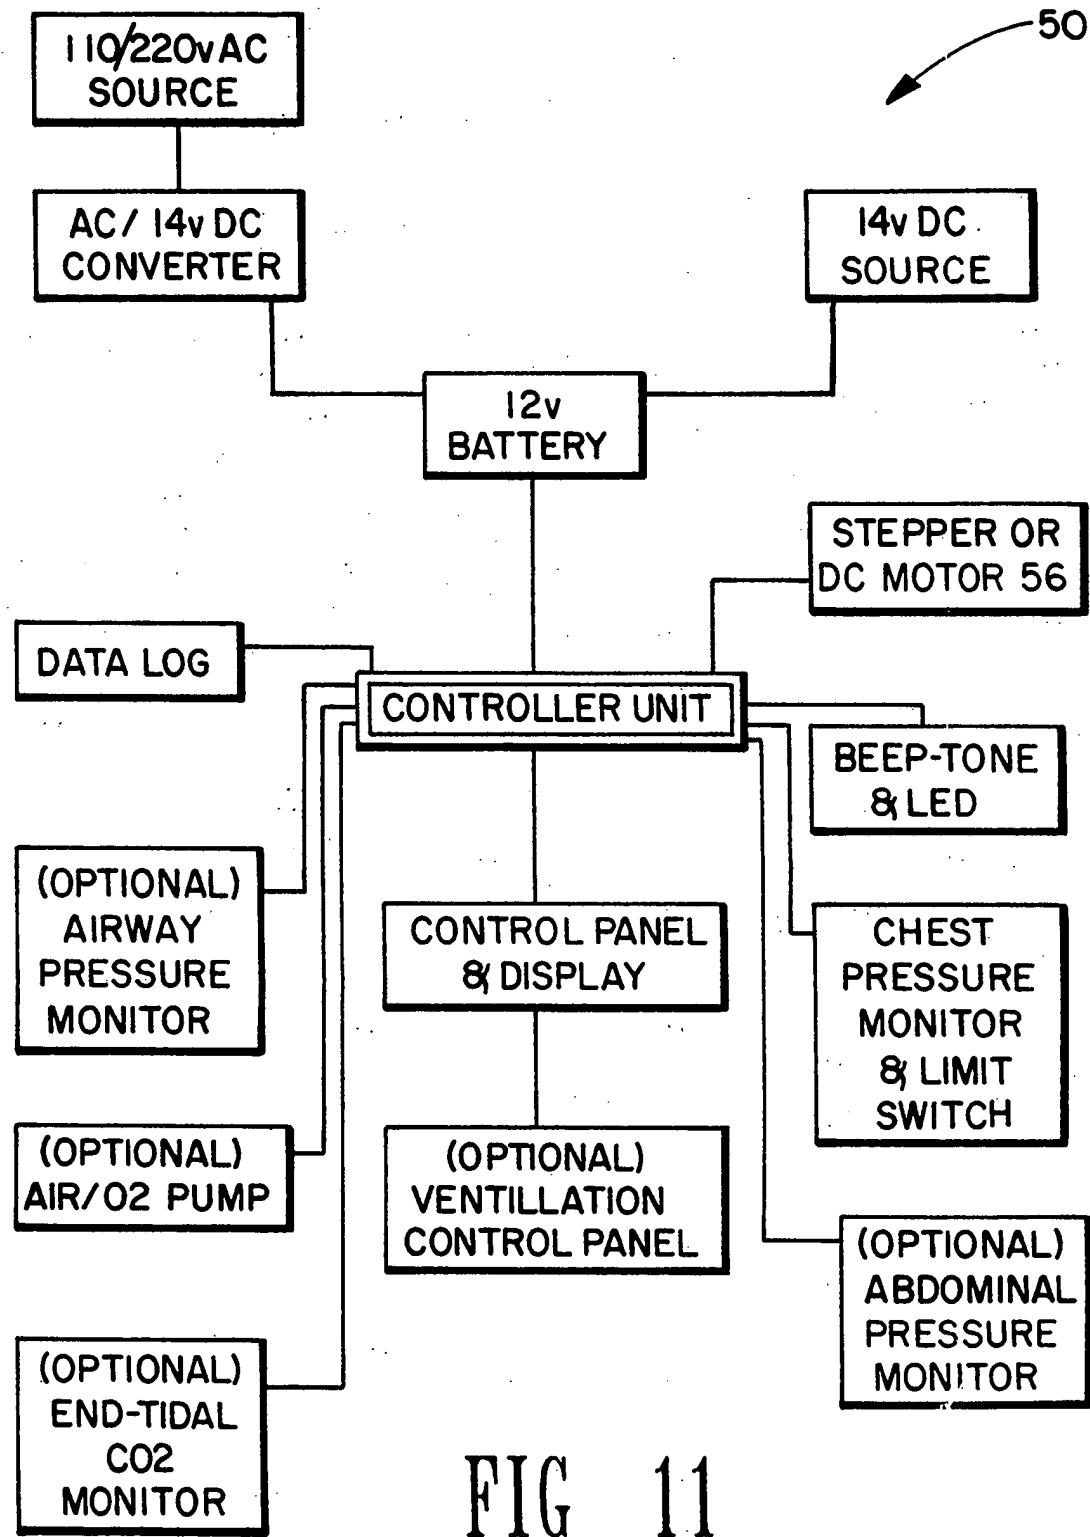


FIG 11

10/15

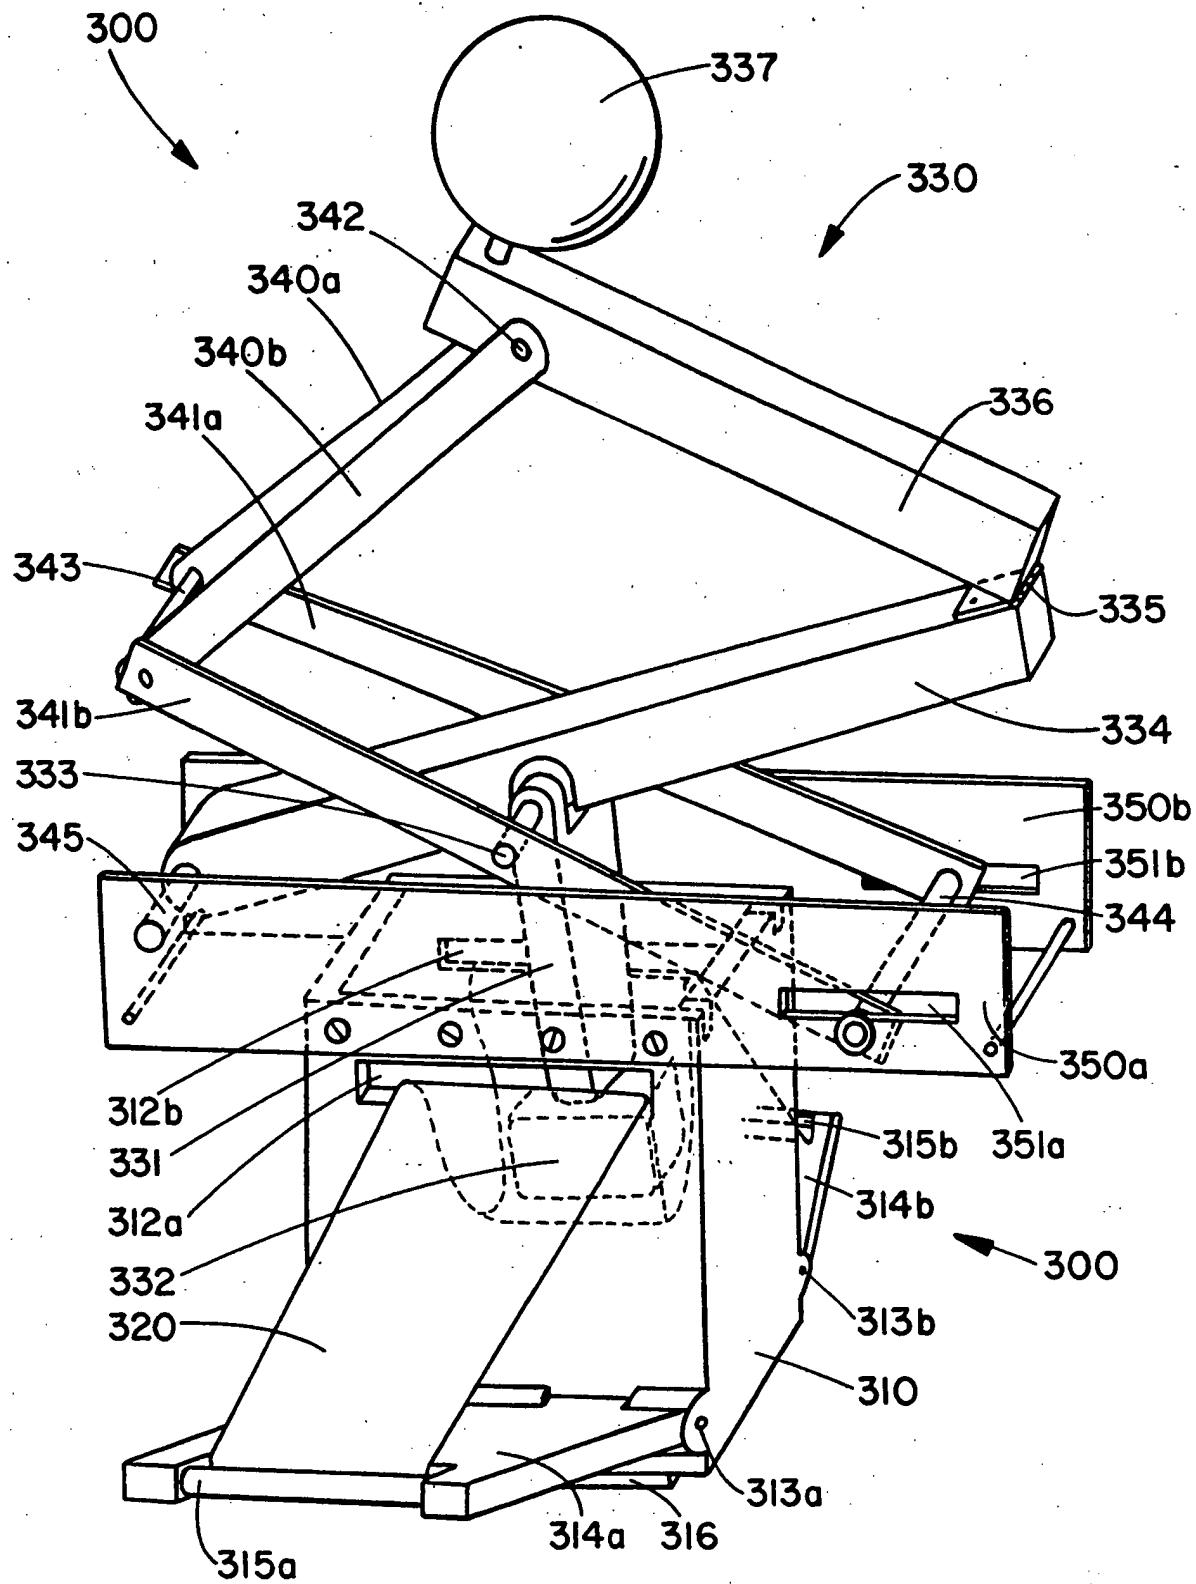


FIG. 12

11/15

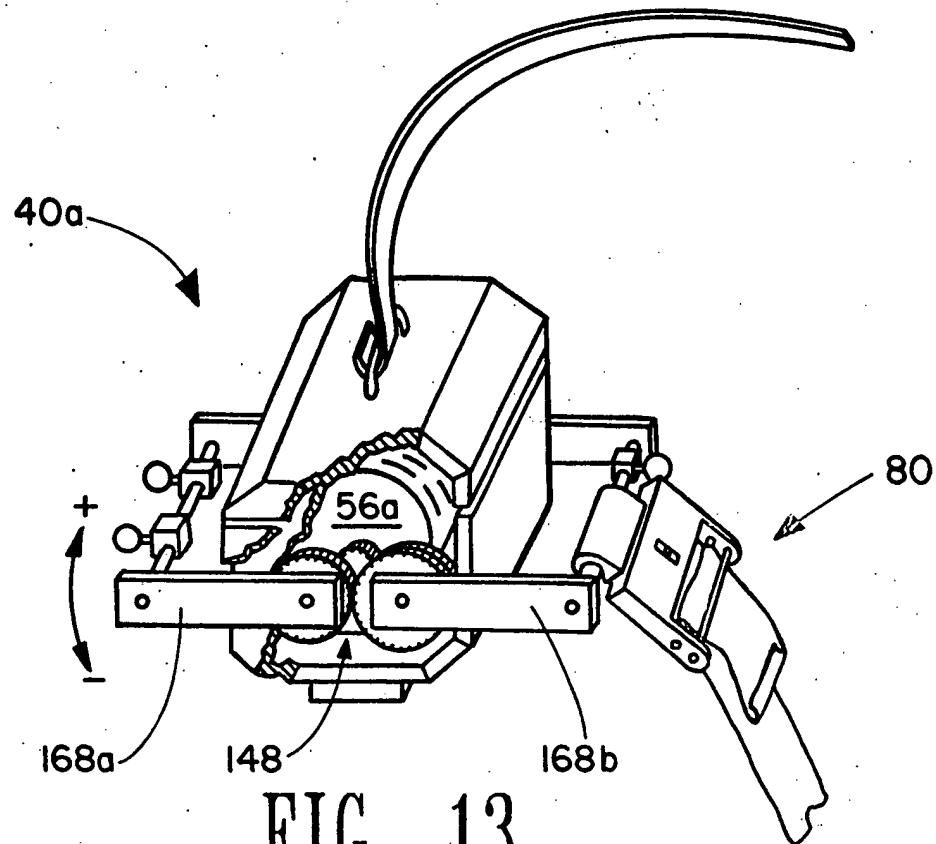


FIG. 13

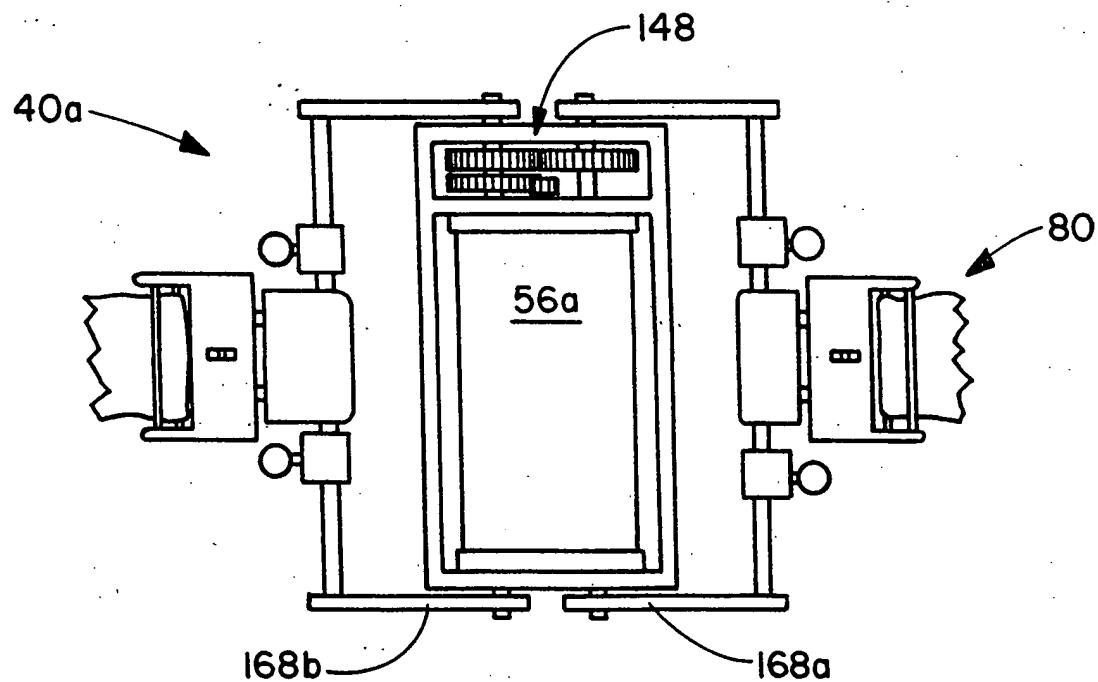


FIG 14

12/15

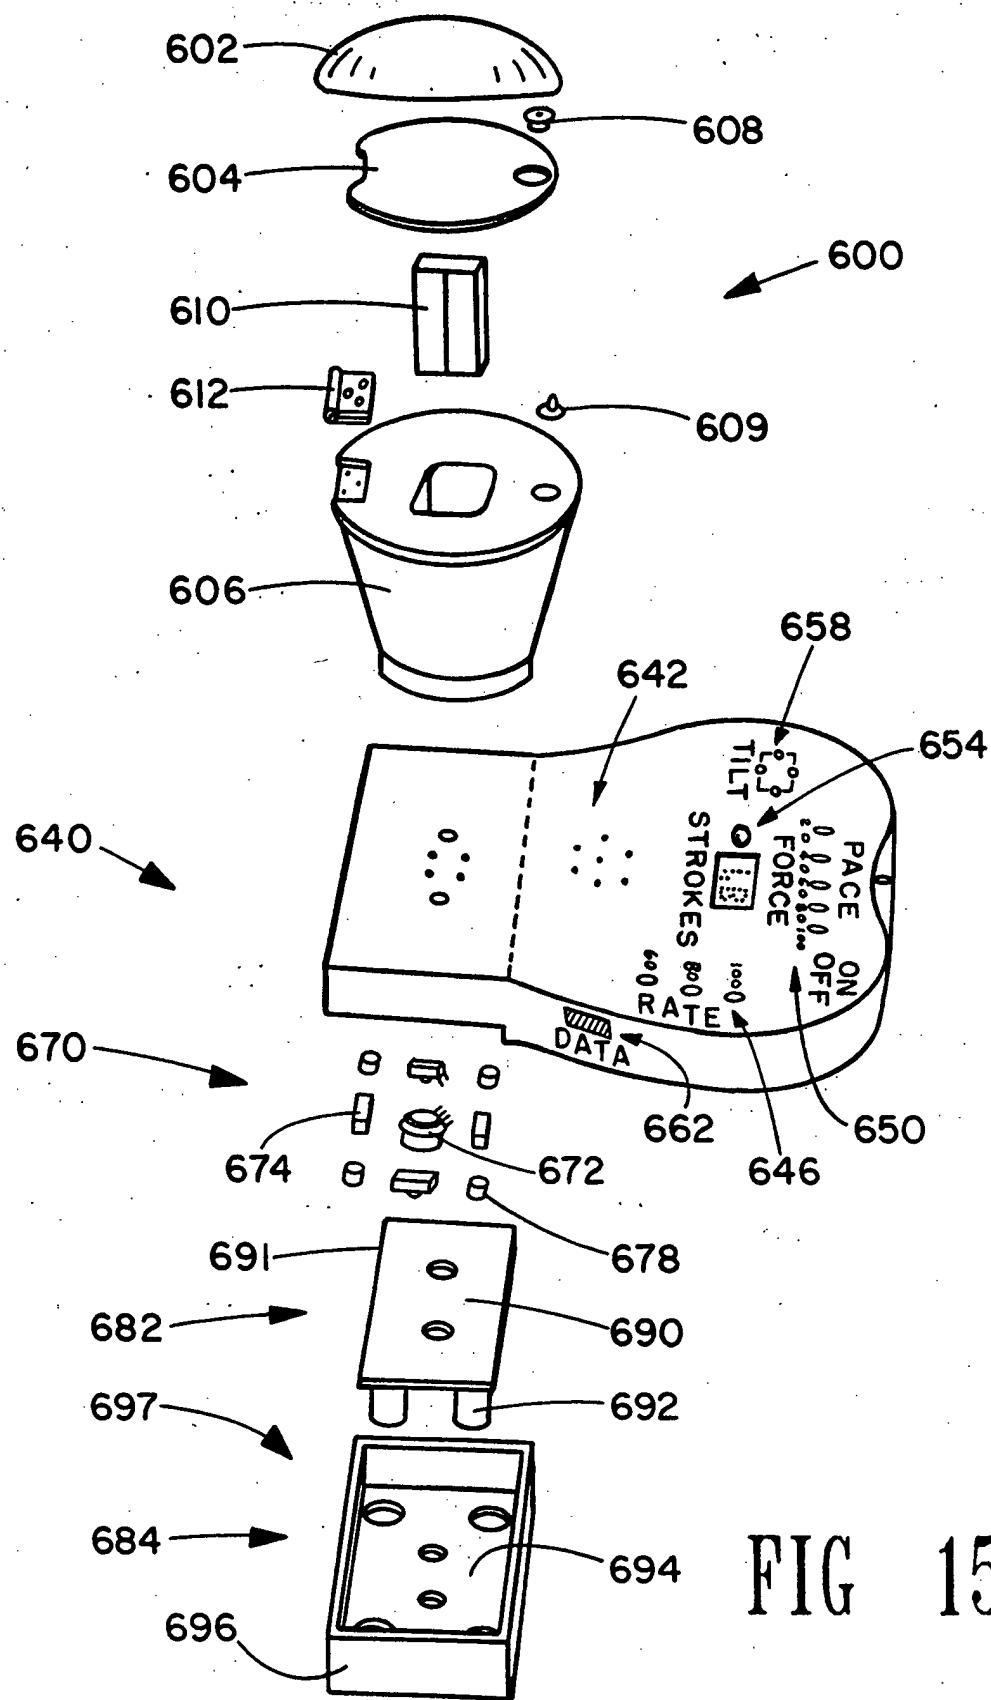


FIG 15

13/15

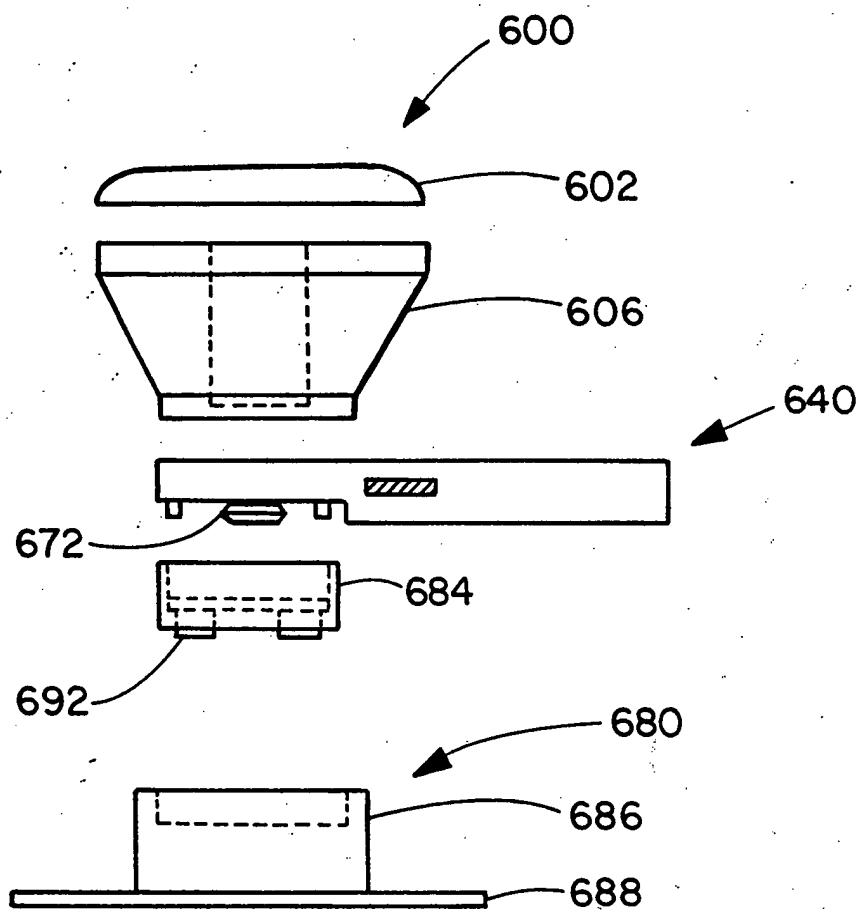


FIG. 16

14/15

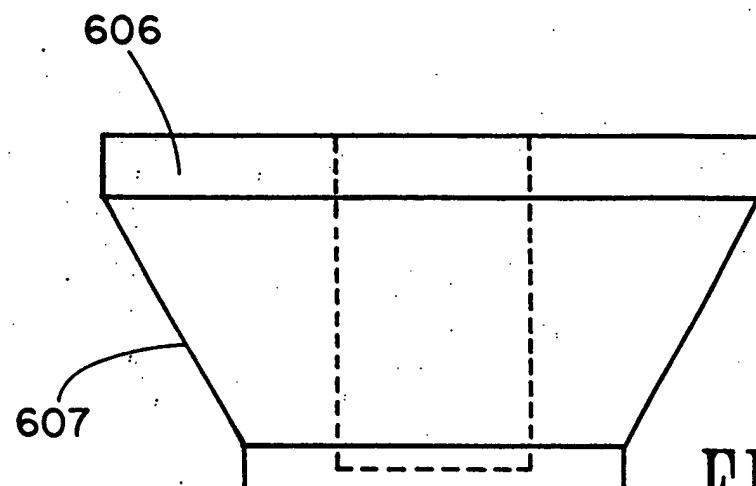


FIG. 17

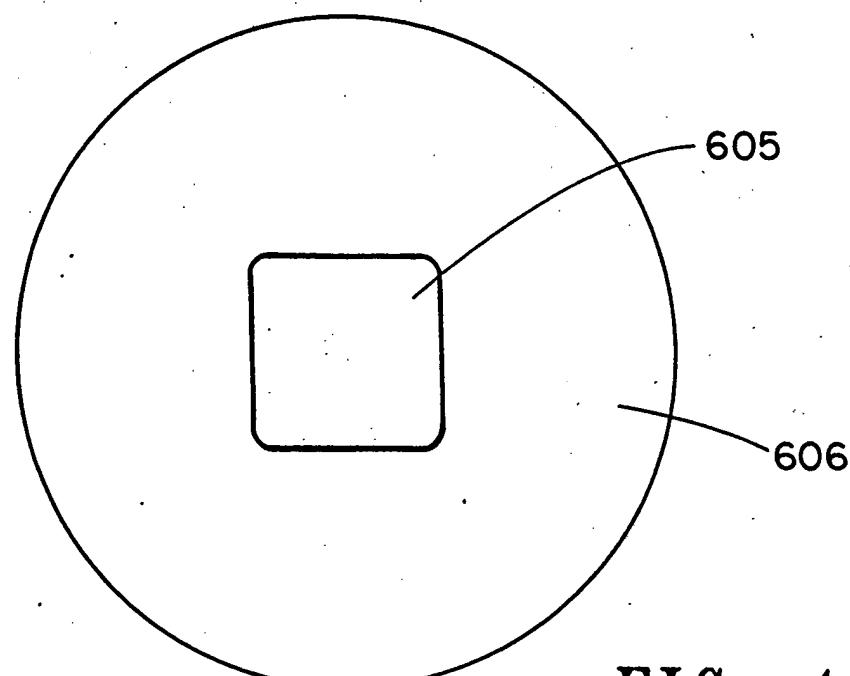


FIG. 18

15/15

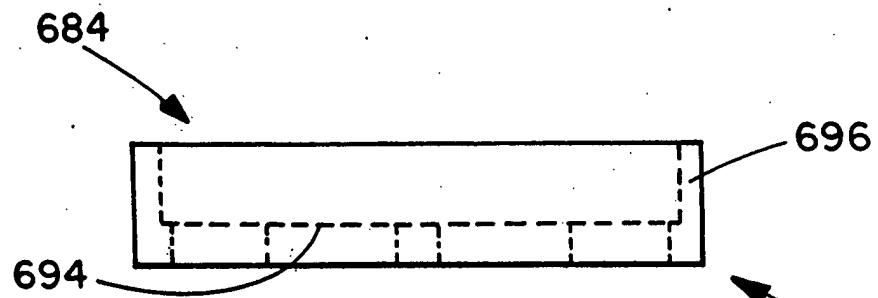


FIG. 19

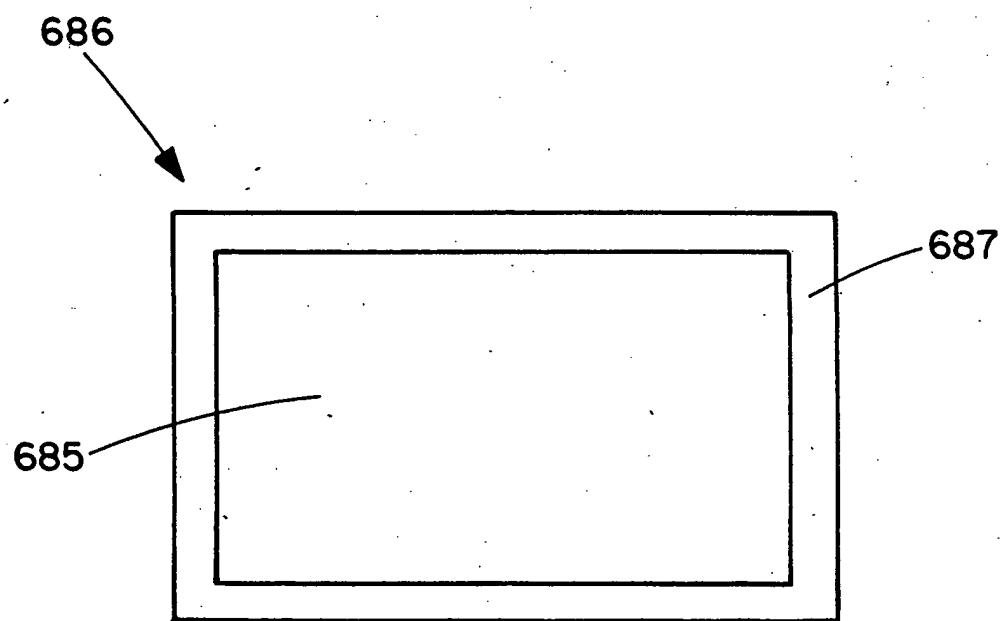


FIG 20